

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXD-0004
Location:	SPRING LAKE HEIGHTS PD	
Calibration File No.:	00336	Calib. Date: 02/26/2018
Certification File No.:	00337	Calib. No.: 00026
Linearity File No.:	00338	Cert. Date: 02/26/2018
Solution File No.:	00341	Cert. No.: 00023
Sequential File No.:	00341	Lin. Date: 02/26/2018
		Lin. No.: 00025
		Soln. Date: 03/28/2018
		Soln. No.: 00127
		File Date: 03/28/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDZJ-0097
Solution Control Lot:	17420	Expires: 12/11/2019
		Bottle No.: 0179

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:38S		
Control 1 EC	0.100%	02:38S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	02:38S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:39S		
Control 2 EC	0.097%	02:40S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:40S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:41S		
Control 3 EC	0.097%	02:41S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	02:41S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RAMP

First Name: ZACHARY

MI: M

Signature: _____

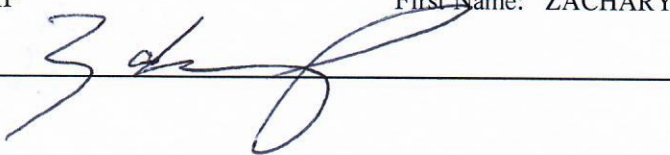

Badge No.: 4926

Date: 03/28/2018