

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXD-0004
Location:	SPRING LAKE HEIGHTS PD	
Calibration File No.:	00364	Calib. Date: 01/29/2019
Certification File No.:	00365	Cert. No.: 00028
Linearity File No.:	00366	Cert. Date: 01/29/2019
Solution File No.:	00369	Lin. No.: 00025
Sequential File No.:	00369	Lin. Date: 01/29/2019
		Soln. No.: 00140
		Soln. Date: 03/31/2019
		File Date: 03/31/2019

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDZJ-0097
Control Solution %: 0.100%		Expires: 12/11/2019
Solution Control Lot: 17420		Bottle No.: 0285

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:28S		
Control 1 EC	0.101%	19:28S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:29S		
Control 2 EC	0.099%	19:30S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	19:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:31S		
Control 3 EC	0.099%	19:32S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	19:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: RAMP

First Name: ZACHARY

MI: M

Signature:

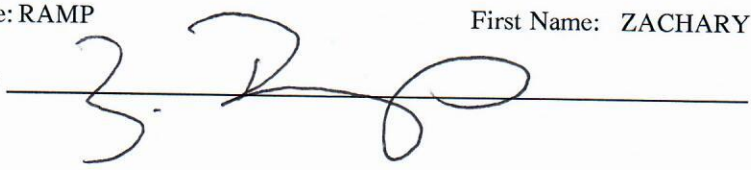

Badge No.: 4926

Date: 03/31/2019