

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXD-0004
Location:	SPRING LAKE HEIGHTS PD	
Calibration File No.:	00364	Calib. Date: 01/29/2019
Certification File No.:	00365	Cert. No.: 00028
Linearity File No.:	00366	Cert. No.: 00025
Solution File No.:	00371	Lin. No.: 00027
Sequential File No.:	00371	Soln. No.: 00141
		File Date: 05/06/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDZJ-0097
Solution Control Lot:	17420	Expires: 12/11/2019
		Bottle No.: 0578

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:45D		
Control 1 EC	0.103%	18:46D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:46D		
Control 2 EC	0.101%	18:47D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	18:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:48D		
Control 3 EC	0.101%	18:49D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RAMP

First Name: ZACHARY

MI: M

Signature: _____

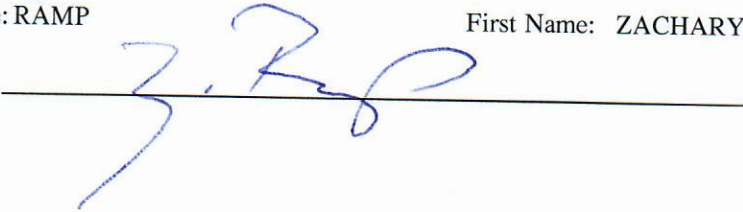

Badge No.: 4926

Date: 05/06/2019