

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXD-0004
Location:	SPRING LAKE HEIGHTS PD	
Calibration File No.:	00364	Calib. Date: 01/29/2019
Certification File No.:	00365	Cert. No.: 00028
Linearity File No.:	00366	Cert. Date: 01/29/2019
Solution File No.:	00373	Lin. No.: 00025
Sequential File No.:	00373	Lin. Date: 01/29/2019
		Soln. No.: 00142
		Soln. Date: 05/27/2019
		File Date: 05/27/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDZJ-0097
Solution Control Lot:	17420	Expires: 12/11/2019
		Bottle No.: 0062

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:33D		
Control 1 EC	0.100%	23:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	23:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:35D		
Control 2 EC	0.100%	23:35D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	23:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:36D		
Control 3 EC	0.099%	23:37D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	23:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: RAMP

First Name: ZACHARY

MI: M

Signature: \_\_\_\_\_

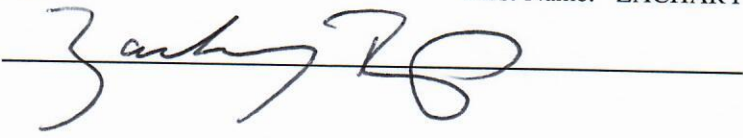

Badge No.: 4926

Date: 05/27/2019