

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXD-0004
Location: SPRING LAKE HEIGHTS PD
Calibration File No.: 00336 Calib. Date: 02/26/2018 Calib. No.: 00026
Certification File No.: 00337 Cert. Date: 02/26/2018 Cert. No.: 00023
Linearity File No.: 00338 Lin. Date: 02/26/2018 Lin. No.: 00025
Solution File No.: 00344 Soln. Date: 05/30/2018 Soln. No.: 00129
Sequential File No.: 00344 File Date: 05/30/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDZJ-0097
Control Solution %: 0.100% Expires: 12/11/2019
Solution Control Lot: 17420 Bottle No.: 0462

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:31D		
Control 1 EC	0.098%	18:32D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	18:32D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:32D		
Control 2 EC	0.097%	18:33D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	18:33D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:34D		
Control 3 EC	0.097%	18:35D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	18:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RAMP

First Name: ZACHARY

MI: M

Signature: _____

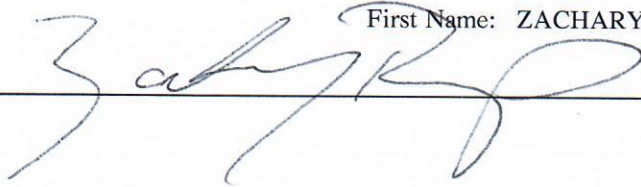

Badge No.: 4926

Date: 05/30/2018