


STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENTATION SERVICE REPORT

| | | |
|--|--|--|
| 1. Department: Spring Lake Heights Police Department 555 Brighton Ave. Spring Lake Heights, NJ 07762 | 2. Contact: Zach Ramp 3. Phone Number: 732-449-6161 | 4. Date: 01/02/2020 5. County: Monmouth |
| 6. Alcotest Instrument Serial Number: ARXD-0004 | 7. Simulator Component Serial Number: N/A | 8. Temperature Probe Component Serial Number: N/A |

9. Reason for Service:
The alcotest instrument was returned from outside evaluation and placed back in service.

10. Comments:
See Draeger Return and Repair form.

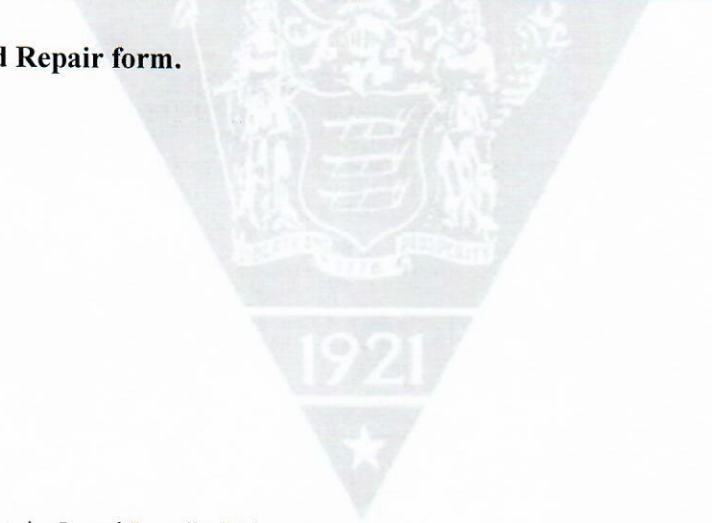


Last Known Sequential File #: NA

- 11. The above Instrument/Component has been found to be in satisfactory working condition; no further action required.
- 12. The above Instrument/Component is placed out of service pending further evaluation.
- 13. The above Instrument/Component is placed back in service.

"I have been certified by the Attorney General as a Breath Test Coordinator/Instructor pursuant to N.J.A.C. 13:51, et. seq. In my official capacity as a Breath Test Coordinator/Instructor I perform inspections of evidential breath test devices and related components of evidential breath test systems. I have inspected the evidential breath test device listed on this report in my official capacity. The results of my inspection are recorded on this form. I certify that the forgoing statements made by me are true and accurate to the best of my knowledge. I am aware that if any of the forgoing statements made by me are willingly false, I am subject to punishment."

Tpr. I Dennis Lutz #7045
 Name & Badge Number (Print)



 Signature 1-2-20
 Date

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENTATION SERVICE REPORT

| | | |
|--|--|--|
| 1. Department: Spring Lake Heights Police Department 555 Brighton Ave. Spring Lake Heights, NJ 07762 | 2. Contact: Zach Ramp 3. Phone Number: 732-449-6161 | 4. Date: 10/18/19 5. County: Monmouth |
| 6. Alcotest Instrument Serial Number: ARXD-0004 | 7. Simulator Component Serial Number: N/A | 8. Temperature Probe Component Serial Number: N/A |

9. Reason for Service:
Complaint received of the inability to remotely connect to the Alcotest instrument on (3) three separate occasions while attempting to retrieve data.

10. Comments:
Operational condition of the instrument was assessed by confirming that the dedicated phone line was functioning properly. A separate test instrument was connected to the dedicated phone line and the test instrument remotely connected and successfully retrieved data.

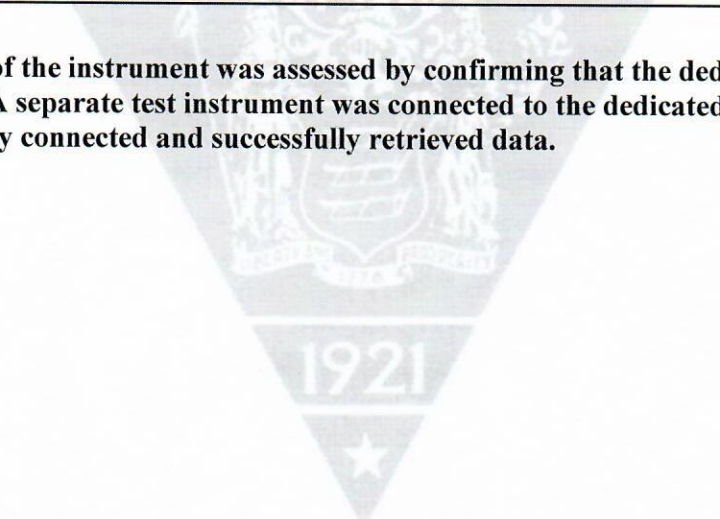


Last Known Sequential File #: 388

- 11. The above Instrument/Component has been found to be in satisfactory working condition; no further action required.
- 12. The above Instrument/Component is placed out of service pending further evaluation.
- 13. The above Instrument/Component is placed back in service.

"I have been certified by the Attorney General as a Breath Test Coordinator/Instructor pursuant to N.J.A.C. 13:51, et. seq. In my official capacity as a Breath Test Coordinator/Instructor I perform inspections of evidential breath test devices and related components of evidential breath test systems. I have inspected the evidential breath test device listed on this report in my official capacity. The results of my inspection are recorded on this form. I certify that the forgoing statements made by me are true and accurate to the best of my knowledge. I am aware that if any of the forgoing statements made by me are willingly false, I am subject to punishment."

Tpr. I Dennis Lutz #7045
Name & Badge Number (Print)

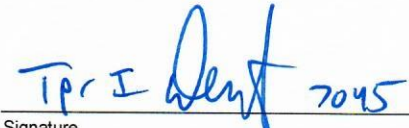
Signature

10-18-19
Date

RETURN AND REPAIR FORM



Customer Information

B: _____ S: _____

Company Name: Spring Lake Heights P.D., Spring Lake Heights, New Jersey

Date Received: 12/02/19 Date given to service: 12/02/19

Carrier: FedEx UPS USPS Shipping Method: GRD 3DAY 2DAY
 NDA-PRI NDA-STD

Product: 6510 6810 Serial Number: AR XD-0004
 7110 8610 Printer Serial#: AR
 7510 DT5000 Sim Serial#: DD
 7410 Upper-half 9510 Probe Serial#: DD
 7410 Whole

Warranty Expires: _____

Description: A B Plus Demo Screener Trade In

Accessories

110V A/C Adapter Regulator Printer Ribbon Printer Paper
 Mouthpieces 9510 Stylus 9510 Top Cover Carrying Case
 Dry Gas Other (please specify) _____

Repair Information

Test#: _____

| Part Number | Description | Qty | Total Cost |
|-------------|---------------|-----|------------|
| MP Cal 71 | Calibration | 1 | |
| MP Labor | Labor | 2 | |
| 6808455 | Fuel Cell | 1 | |
| 6808374 | Geared Engine | 1 | |
| | | | |
| | | | |
| | | | |
| | | | |

Repair Notes: Replaced defective fuel cell, geared engine, c156 and 167.
C156 and C167 was changed to resolve the modem issue that the
customer is having and are non-inventory parts.

FUEL CELL = ARMH-0562
CAL W/QC AND OPS CHECK

Service Technician BS Date: 12/20/19



Delivery receipt



Customer no.
150078002

Number of report
304751658
Please reference on inquiries

Date of receiving Delivery receipt date
/ / 12/20/2019

Consignee, 150078003
SPRING LAKE HEIGHTS POLICE DEPT
ATTN: ZACHARY RAMP
PO# ARXD-0004
555 BRIGHTON AVE
SPRING LAKE HEIGHTS NJ 07762-2093

Customer, 150078002
BOROUGH OF SPRING LAKE HEIGHTS
ATTN; JANINE GILLIS
PO# ARXD-0004
555 BRIGHTON AVE
SPRING LAKE HEIGHTS NJ 07762-2099

Your order

Date of order:
11/21/2019
Purch.ord.no. :
19-01960

Branch text

Draeger contact person

Service Support-IDT
800-437-2437 OPT 5
SS-IDT@draeger.com

Page 1

| Quantity | Description | Part no. | Equipment - No. | Serial - No. |
|----------|--------------------------|----------|-----------------|--------------|
| 001 | ALCOTEST 7110 MK III USA | 8314246 | 1029324743 | ARXD-0004 |

Draeger Inc.
Our Tax ID: 23-1699096
3135 Quarry Road, Telford, PA 18969
An Equal Opportunity Employer M / F / V / H
Telephone 800-437-2437
<http://www.draeger.com>

Remit to:
LOCKBOX (Standard USPS)
Draeger, Inc.
PO Box 13369
Newark, New Jersey
07101-3362

Remit to:
LOCKBOX (Overnight)
FIS Lockbox Processing
Lockbox #13369
100 Grove Road
Suite E
West Deptford, NJ 08066

Remit US Wire Transfers to:
Account Name: Draeger Inc.
Account Number: 00-494-936
Transit Routing: 021001033
SWIFT: BKTRUS33
Deutsche Bank Trust Company Americas
60 Wall Street 25th Fl, New York, NY 10005

Service note

Customer no. 150078002 Number of report 304751658 Date of receiving 12/16/2019
 Please reference on inquiries

Customer
 BOROUGH OF SPRING LAKE HEIGHTS
 555 BRIGHTON AVE
 SPRING LAKE HEIGHTS NJ 07762-2099

Consignee
 SPRING LAKE HEIGHTS POLICE DEPT
 ATTN: ZACHARY RAMP
 555 BRIGHTON AVE
 SPRING LAKE HEIGHTS NJ 07762-2093

Your order
 Date of order: 11/21/2019
 Your reference: 19-01960

NL-Text
 Maintenance device list

Your contact person
 Service Support-IDT
 800-437-2437 OPT 5
 SS-IDT@draeger.com

Page 1

| Item | Quantity | Part no. Description |
|-------------------------|----------|--|
| | | Service Order: 142279461 |
| | | COE005759 |
| | | Eq.No. : 1029324743 SN: ARXD-0004 |
| | | Material: 8314246 ALCOTEST 7110 MK III USA |
| | | Inv.No. : |
| | | Location: |
| | | COE005759 |
| | 2.0 H | R018 Repair time - Core |
| | 1 EA | 6808455 Sensor Alcotest B |
| | 1 EA | 6808374 Geared Engine, A7110/A9510 |
| | 1 EA | 6808486 Connector, A7110/A9510 |
| <hr/> | | |
| PAPERWORK | | |
| <hr/> | | |
| CALIBRATION 7110 | | |