

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXD-0004
Location: SPRING LAKE HEIGHTS PD
Calibration File No.: 00398 Calib. Date: 04/27/2020 Calib. No.: 00032
Certification File No.: 00399 Cert. Date: 04/27/2020 Cert. No.: 00028
Linearity File No.: 00400 Lin. Date: 04/27/2020 Lin. No.: 00030
Solution File No.: 00404 Soln. Date: 06/14/2020 Soln. No.: 00153
Sequential File No.: 00404 File Date: 06/14/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDZJ-0097
Control Solution %: 0.100% Expires: 10/30/2021
Solution Control Lot: 19300 Bottle No.: 0794

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 20:50D | | |
| Control 1 EC | 0.098% | 20:51D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.098% | 20:51D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:51D | | |
| Control 2 EC | 0.098% | 20:52D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.098% | 20:52D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:53D | | |
| Control 3 EC | 0.098% | 20:53D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.097% | 20:53D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:54D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RAMP

First Name: ZACHARY

MI: M

Signature: _____

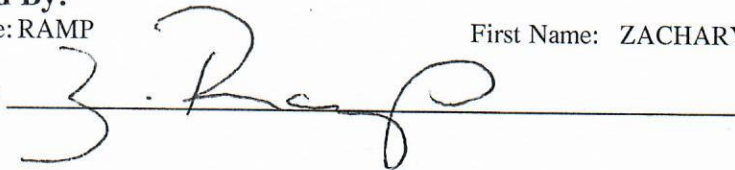

Badge No.: 4926

Date: 06/14/2020