

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXD-0004
Location:	SPRING LAKE HEIGHTS PD	
Calibration File No.:	00412	Calib. Date: 07/28/2020
Certification File No.:	00413	Calib. No.: 00033
Linearity File No.:	00414	Cert. Date: 07/28/2020
Solution File No.:	00427	Cert. No.: 00029
Sequential File No.:	00427	Lin. Date: 07/28/2020
		Lin. No.: 00031
		Soln. Date: 10/05/2020
		Soln. No.: 00158
		File Date: 10/05/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDZI-0097
Solution Control Lot:	20180	Expires: 03/30/2022
		Bottle No.: 0474

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:06D		
Control 1 EC	0.102%	21:06D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	21:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:07D		
Control 2 EC	0.101%	21:08D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	21:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:08D		
Control 3 EC	0.102%	21:09D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	21:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:10D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: RAMP

First Name: ZACHARY

MI: M

Signature: \_\_\_\_\_

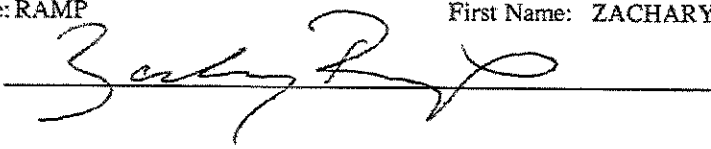

Badge No.: 4926

Date: 10/05/2020