

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXD-0004
Location: SPRING LAKE HEIGHTS PD
Calibration File No.: 00433 Calib. Date: 01/13/2021 Calib. No.: 00034
Certification File No.: 00434 Cert. Date: 01/13/2021 Cert. No.: 00030
Linearity File No.: 00435 Lin. Date: 01/13/2021 Lin. No.: 00032
Solution File No.: 00441 Soln. Date: 03/29/2021 Soln. No.: 00165
Sequential File No.: 00441 File Date: 03/29/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDZJ-0096
Control Solution %: 0.100% Expires: 10/21/2022
Solution Control Lot: 20460 Bottle No.: 1119

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:00S		
Control 1 EC	0.095%	19:00S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	19:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:01S		
Control 2 EC	0.095%	19:02S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	19:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:03S		
Control 3 EC	0.095%	19:03S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	19:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:04S		

All tests within acceptable tolerance.

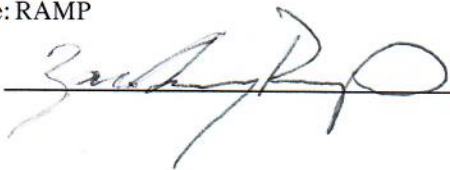
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: RAMP

First Name: ZACHARY

MI: M

Signature: 

Badge No.: 4926

Date: 03/29/2021