

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARXD-0004
Location:	SPRING LAKE HEIGHTS PD		
Calibration File No.:	00464	Calib. Date:	12/28/2021
Certification File No.:	00465	Cert. No.:	00036
Linearity File No.:	00466	Cert. Date:	12/28/2021
Solution File No.:	00473	Lin. No.:	00034
Sequential File No.:	00473	Lin. Date:	12/28/2021
		Soln. Date:	04/19/2022
		Soln. No.:	00179
		File Date:	04/19/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDZJ-0096
Solution Control Lot:	22070	Expires:	02/17/2024
		Bottle No.:	0487

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:26D		
Control 1 EC	0.099%	16:27D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:28D		
Control 2 EC	0.099%	16:29D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:29D		
Control 3 EC	0.100%	16:30D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:31D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: DAVIS

First Name: IAN

MI: G

Signature: \_\_\_\_\_

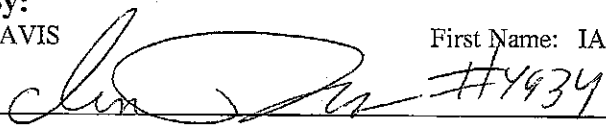

Badge No.: 4934

Date: 04/19/2022